Bioengineering 280A
Principles of Biomedical Imaging

Fall Quarter 2015
X-Rays Lecture 1

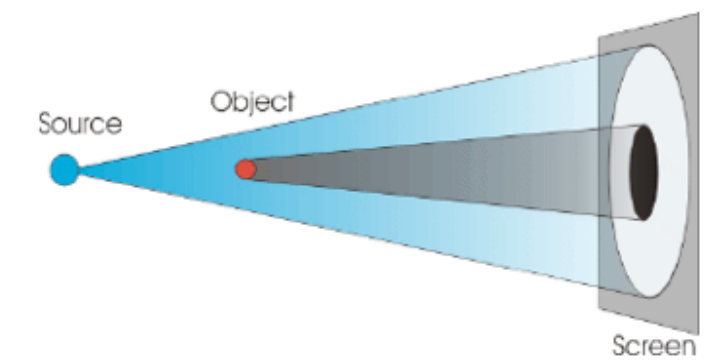

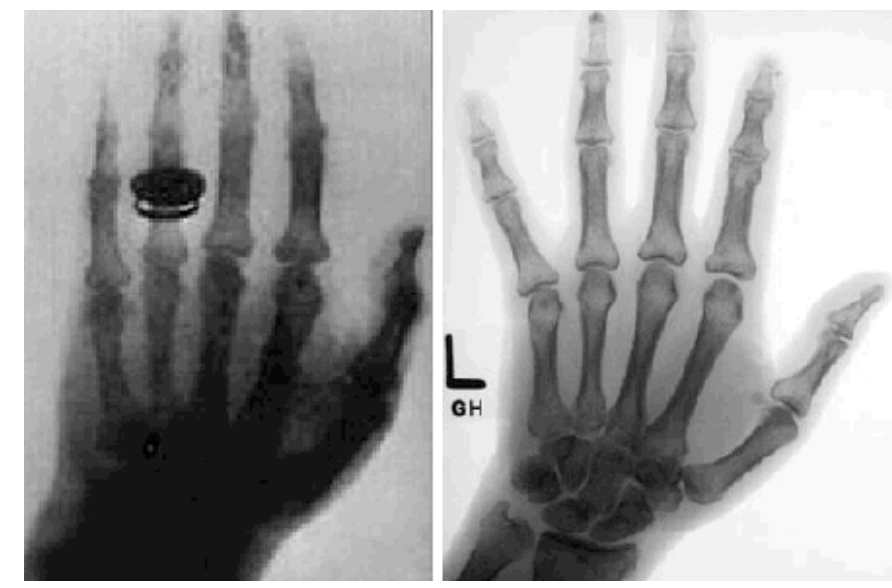

TT Liu, BE280A, UCSD Fall 2015

EM spectrum

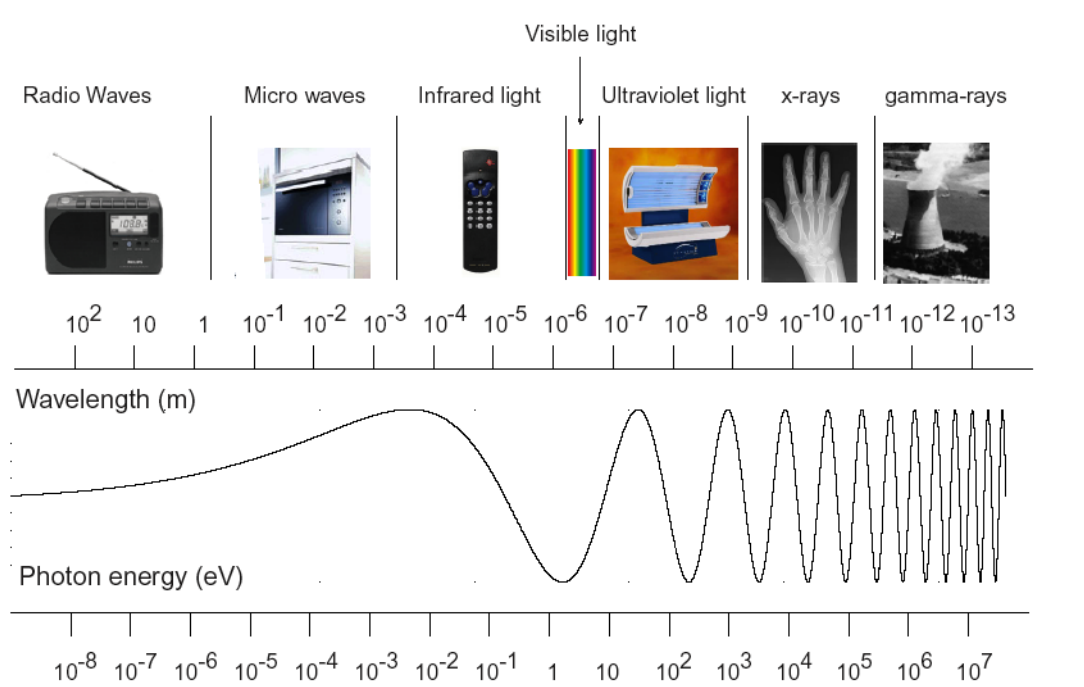

Figure 4.1: *The electromagnetic spectrum.*

Suetens 2002

TT Liu, BE280A, UCSD Fall 2015

http://www.youtube.com/watch?v=wbbsbE2mQuA

TT Liu, BE280A, UCSD Fall 2015

X-Ray Tube

Usually tungsten is used for anode
Molybdenum for mammography

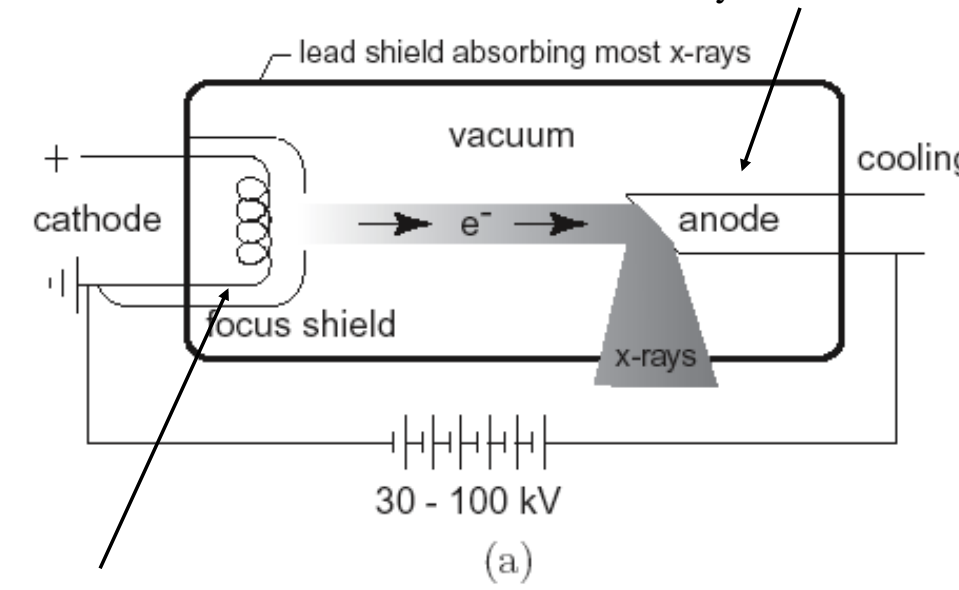

Tungsten filament heated to about 2200 C leading to thermionic emission of electrons.

Suetens 2002

X-Ray Tube

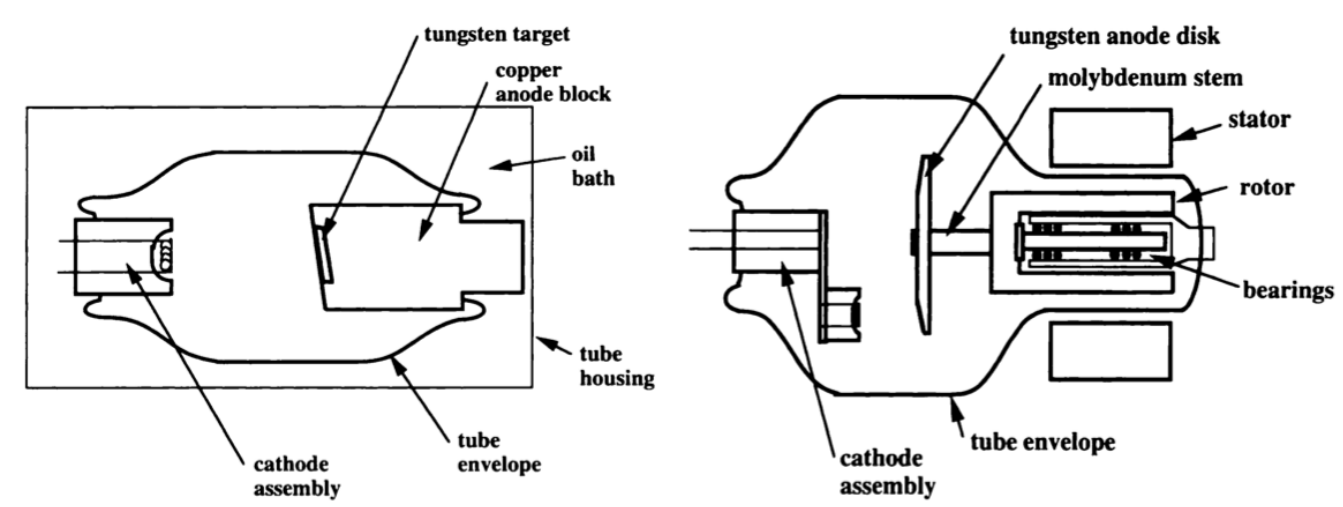

Zink, Radiographics, 1997

X-Ray Production

Collisional transfers

Radiative transfers

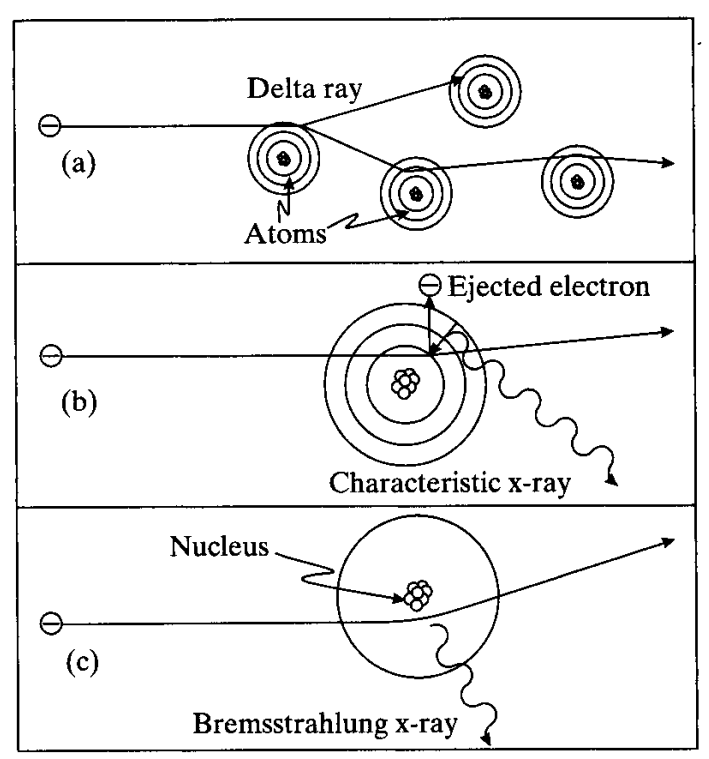

Prince and Links 2005

X-Ray Spectrum

Lower energy photons are absorbed by anode, tube, and other filters

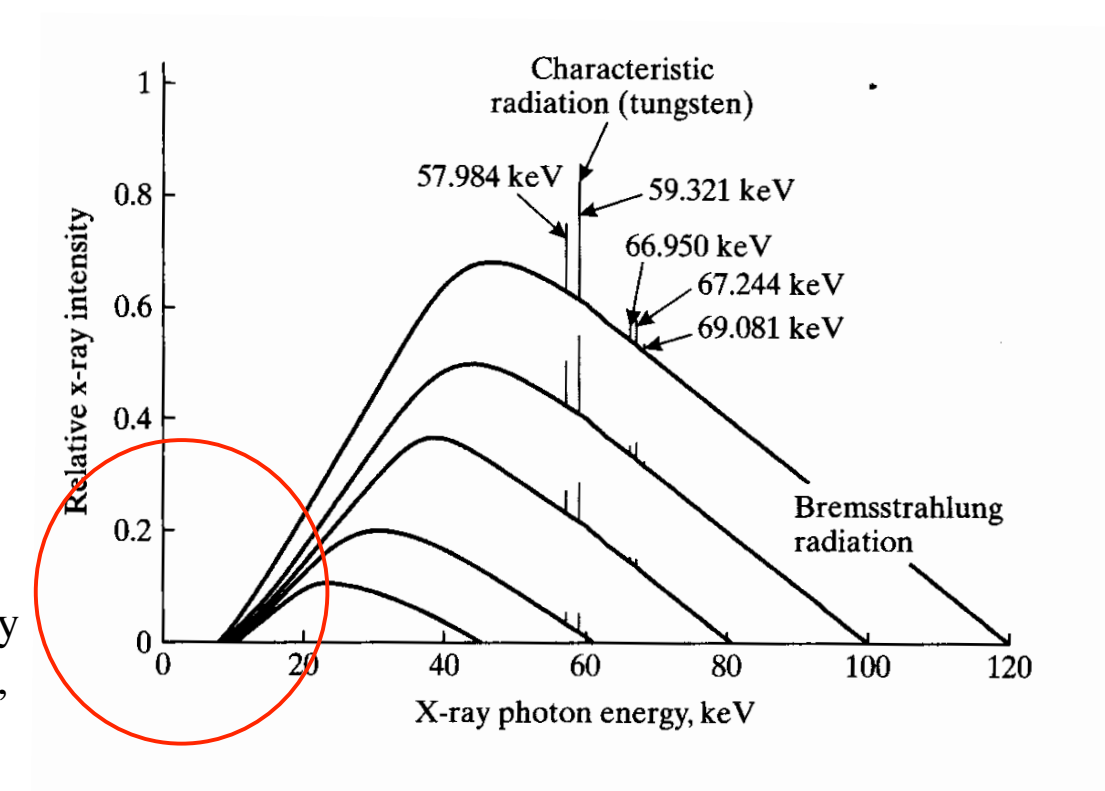

Prince and Links 2005

Interaction with Matter

Typical energy range for diagnostic x-rays is below 200 keV. The two most important types of interaction are photoelectric absorption and Compton scattering.



Photoelectric effect dominates at low x-ray energies and high atomic numbers.

$$E_{e^-} = h\nu - E_B$$

$$\Pr(Event) \propto \frac{Z_{eff}^4}{(h\nu)^3}$$

Compton scattering dominates at high x-ray energies and low atomic numbers, not much contrast



$$\Pr(Event) \propto \frac{N_A Z}{W_m} \approx \text{constant}$$

http://www.eee.ntu.ac.uk/research/vision/asobania

X-Ray Imaging Chain

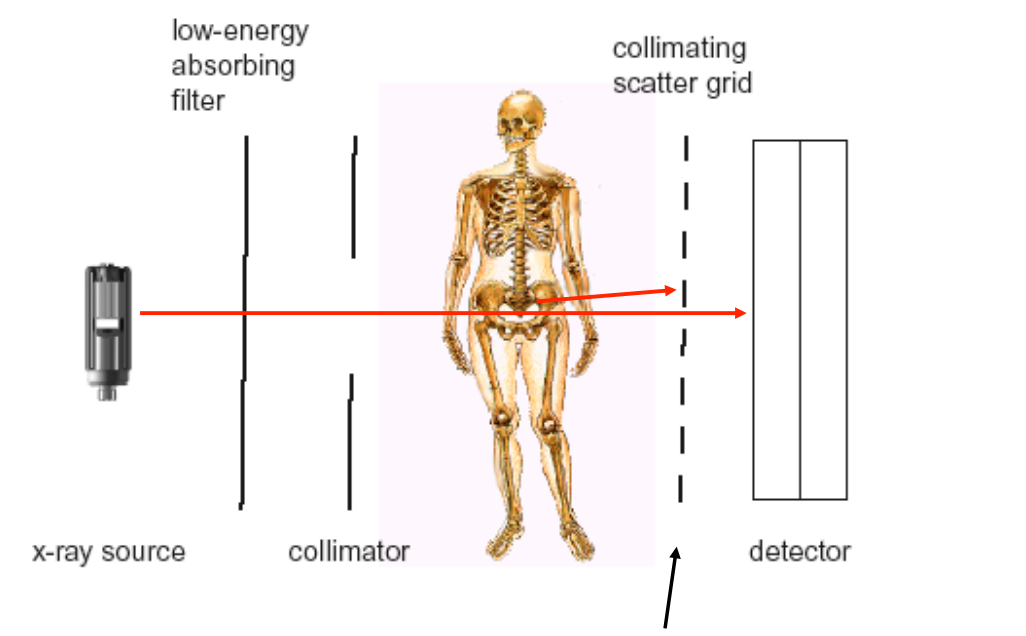

Reduces effects of Compton scattering

Suetens 2002

X-ray film

Emulsion with silver halide crystals
Each layer ~ 10 μm



Flexible base ~ 150 μm

Silver halide crystals absorb optical energy. After development, crystals that have absorbed enough energy are converted to metallic silver and look dark on the screen. Thus, parts in the object that attenuate the x-rays will look brighter.

Intensifying Screen

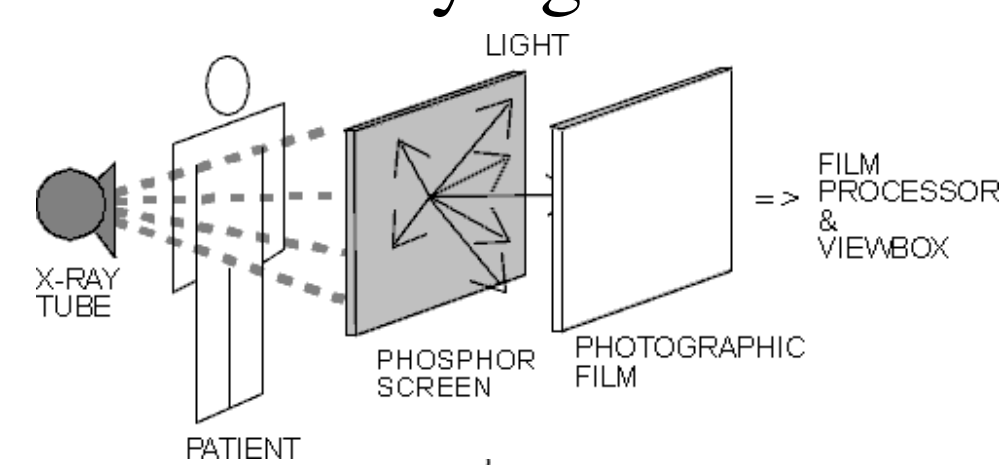

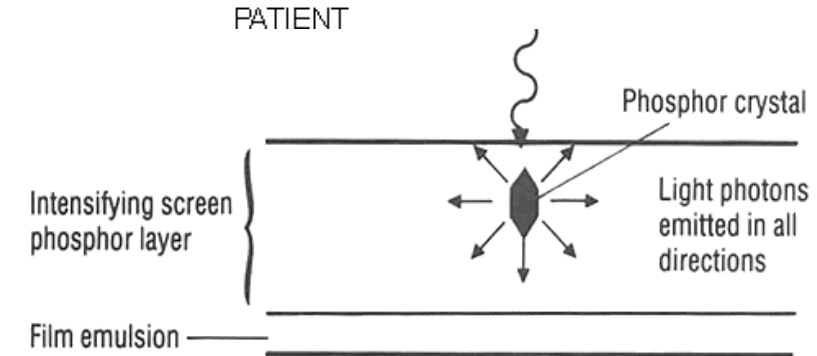

http://learntech.uwe.ac.uk/radiography/RScience/imaging_principles_d/diagimage11.htm
http://www.sunnybrook.utoronto.ca:8080/~selenium/xray.html#Film

Digital Radiography

Table 1
Timetable of Developments in Digital Radiography

Year	Development
1977	Digital subtraction angiography
1980	Computed radiography (CR), storage phosphors
1987	Amorphous selenium–based image plates
1990	Charge-coupled device (CCD) slot-scan direct radiography (DR)
1994	Selenium drum DR
1995	Amorphous silicon–cesium iodide (scintillator) flat-panel detector
1995	Selenium-based flat-panel detector
1997	Gadolinium-based (scintillator) flat-panel detector
2001	Gadolinium-based (scintillator) portable flat-panel detector
2001	Dynamic flat-panel detector fluoroscopy–digital subtraction angiography

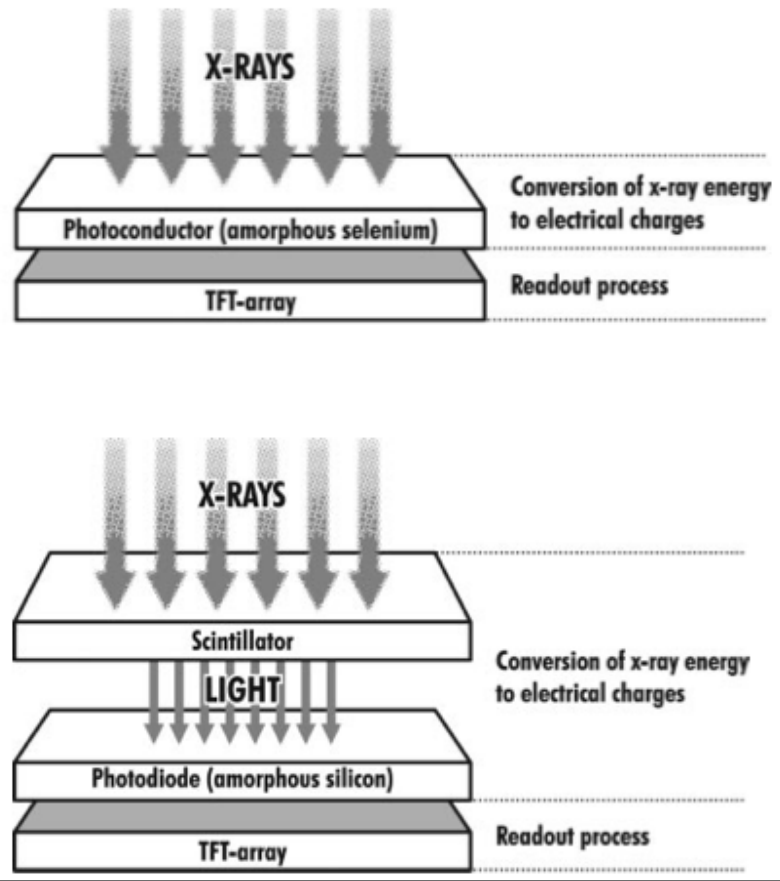

Korner et al, 2007

X-Ray Examples

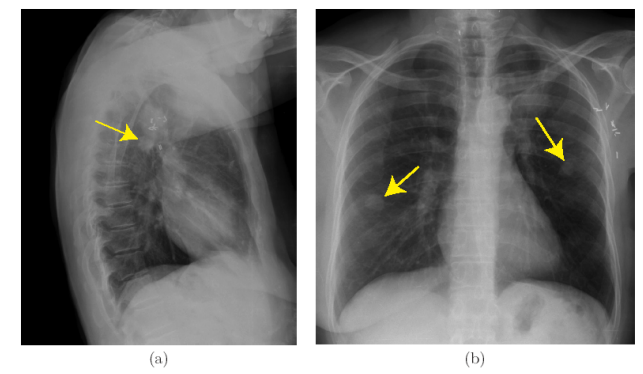

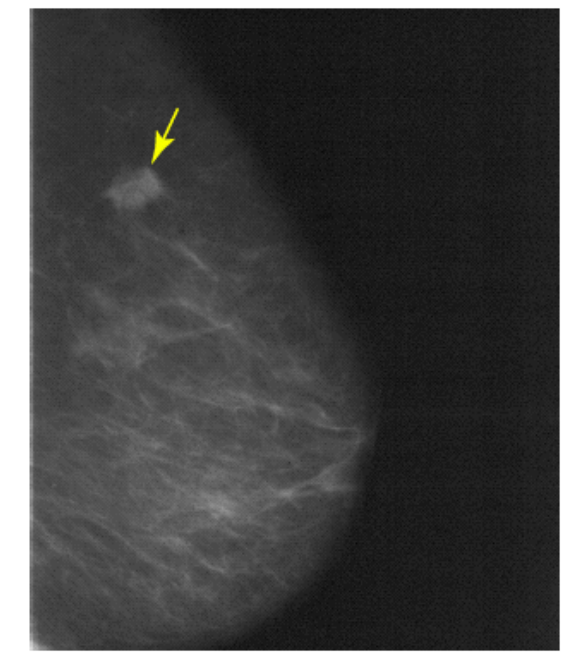

Suetens 2002

http://www.dentistryiq.com/content/dam/diq/online-articles/2013/03/DXRsoftwaresensor.jpg

X-Ray w/ Contrast Agents



Angiogram using an iodine-based contrast agent.
K-edge of iodine is 33.2 keV



Barium Sulfate
K-edge of Barium is 37.4 keV

Suetens 2002

Intensity

$$I = E\phi$$

Energy (E) — Photon flux rate (ϕ)

$$\phi = \frac{N}{A\Delta t}$$

Number of photons (N)

Unit Area (A) — Unit Time (Δt)

Intensity

$$\phi = \int_0^\infty S(E')dE'$$

X-ray spectrum

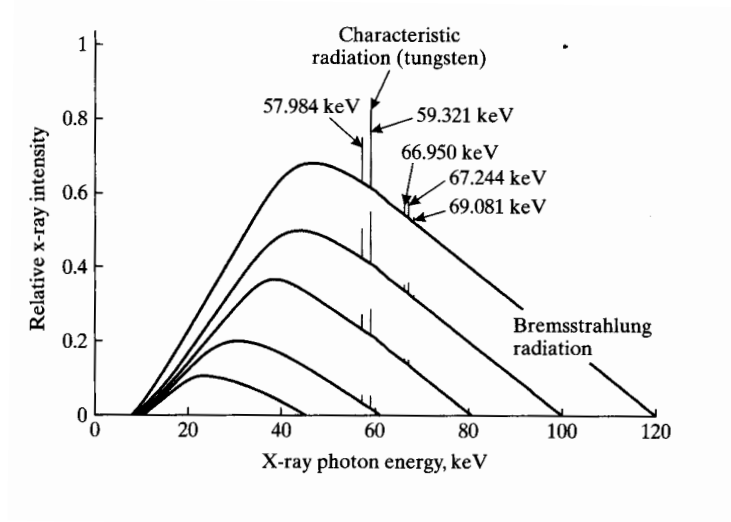

$$I = \int_0^\infty S(E')E'dE'$$

Attenuation

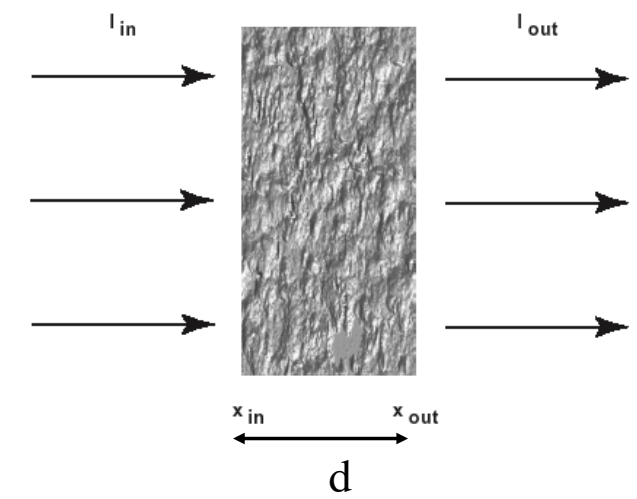

For single-energy x-rays passing through a homogenous object:

$$I_{out} = I_{in}\exp(-\mu d)$$

Linear attenuation coefficient

Attenuation

$n = \mu N \Delta x$ photons lost per unit length

$\mu = \frac{n/N}{\Delta x}$ fraction of photons lost per unit length

$$\Delta N = -n \longrightarrow \frac{dN}{dx} = -\mu N \longrightarrow N(x) = N_0 e^{-\mu x}$$

For mono-energetic case, intensity is

$$I(\Delta x) = I_0 e^{-\mu \Delta x}$$

Attenuation

Inhomogeneous Slab

$$\frac{dN}{dx} = -\mu(x)N \longrightarrow N(x) = N_0 \exp\left(-\int_0^x \mu(x')dx'\right)$$

$$I(x) = I_0 \exp\left(-\int_0^x \mu(x')dx'\right)$$

Attenuation depends on energy, so also need to integrate over energies

$$I(x) = \int_0^\infty S_0(E')E'\exp\left(-\int_0^x \mu(x';E')dx'\right)dE'$$

Contrast

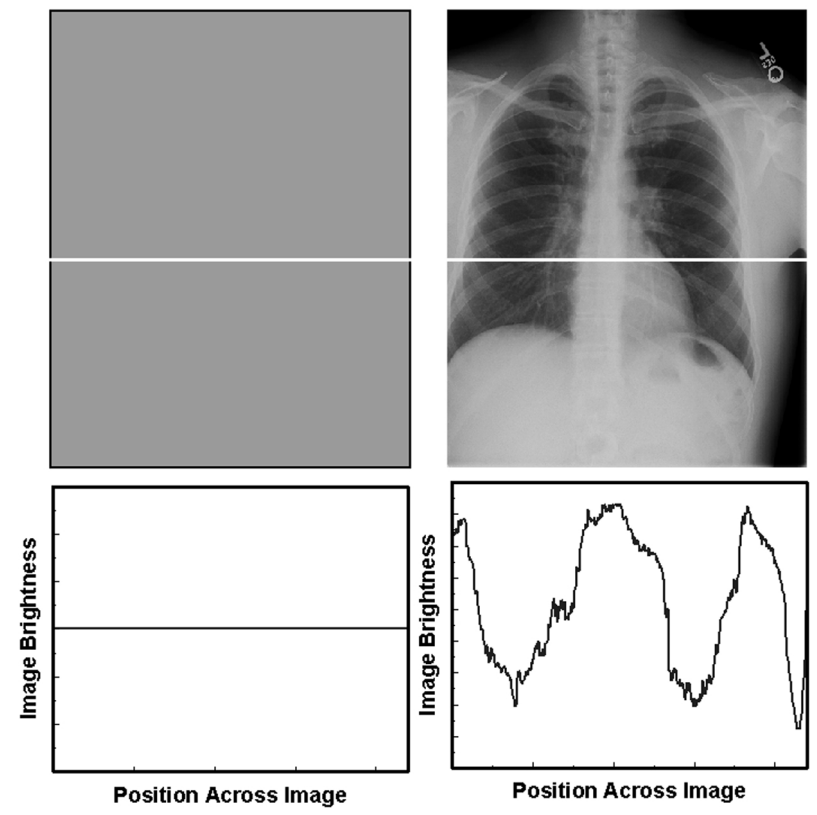

Bushberg et al 2001

Contrast

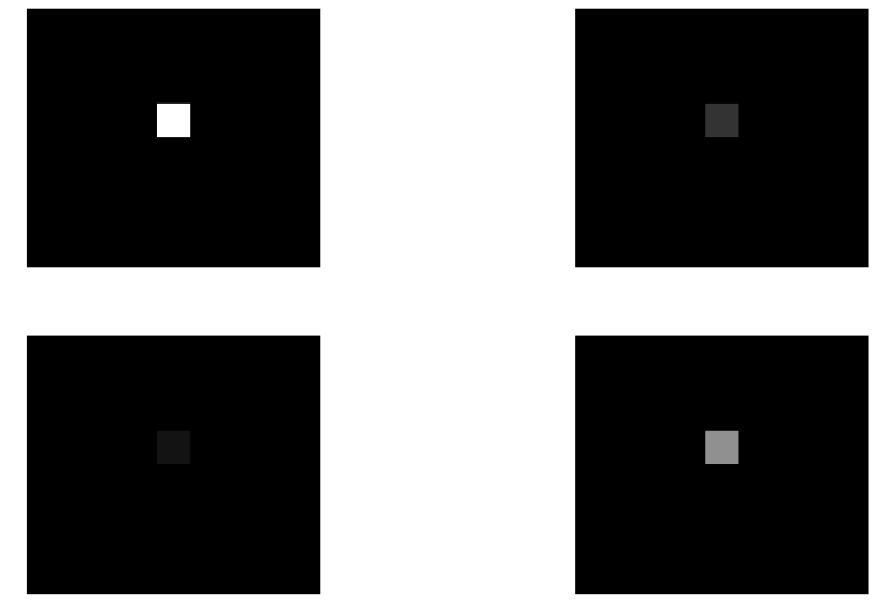

Attenuation

More Attenuation

Attenuation Coefficient

Less Attenuation

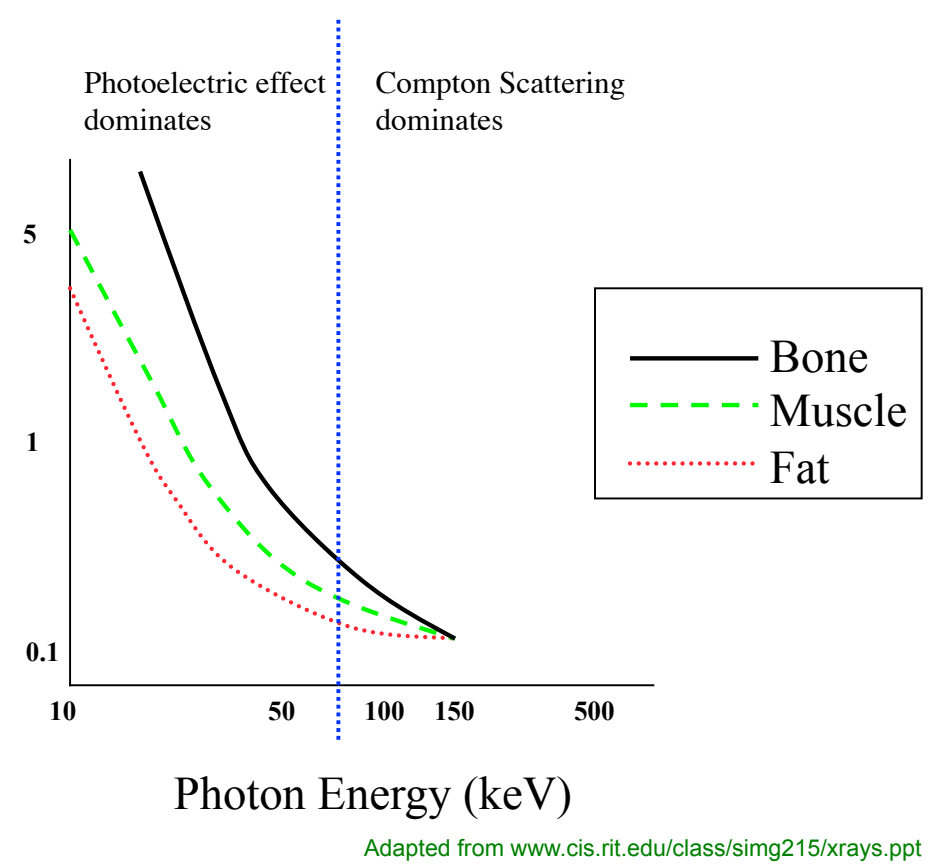

Attenuation

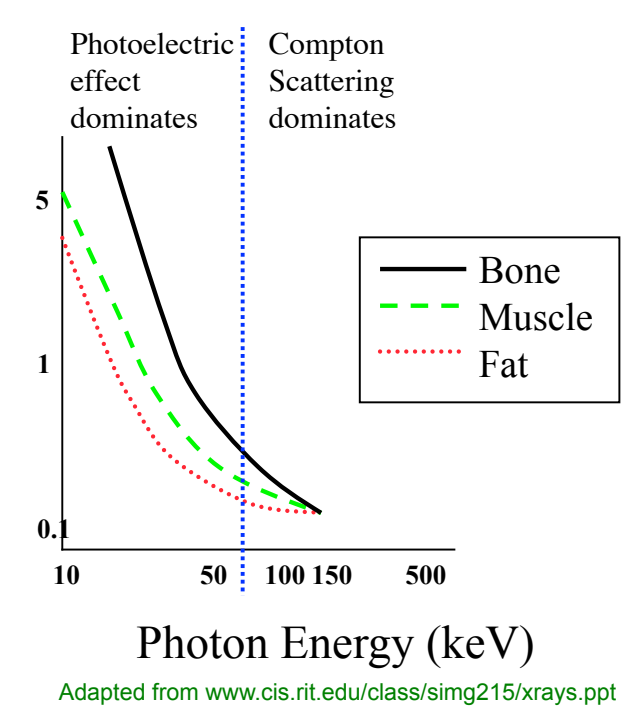

Question: Optimum contrast between Bone and Fat occurs at:

a) 10 keV
b) 20keV
c) 50 keV
d) 100 keV

PollEv.com/be280a

Half Value Layer

X-ray energy (keV)	HVL, muscle (cm)	HVL Bone (cm)
30	1.8	0.4
50	3.0	1.2
100	3.9	2.3
150	4.5	2.8

In chest radiography, about 90% of x-rays are absorbed by body. Average energy from a tungsten source is 68 keV. However, many lower energy beams are absorbed by tissue, so average energy is higher. This is referred to as beam-hardening, and reduces the contrast.

Values from Webb 2003

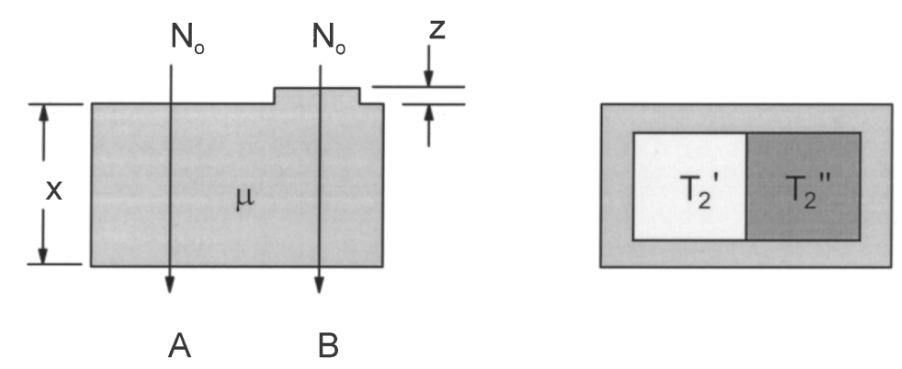

(A) X-ray Imaging

(B) MR Imaging

Bushberg et al 2001

$$A = N_0 \exp(-\mu x)$$
$$B = N_0 \exp(-\mu(x+z))$$

Subject Contrast

$$C_S = \frac{A-B}{A} = \frac{N_0 \exp(-\mu x) - N_0 \exp(-\mu(x+z))}{N_0 \exp(-\mu x)} = 1 - \exp(-\mu z)$$

X-Ray Imaging Geometry

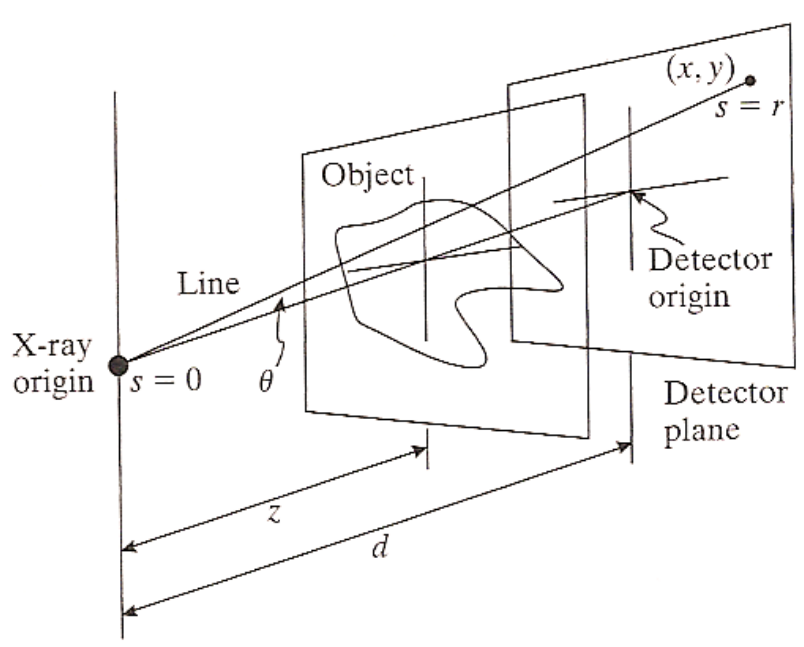

Prince and Links 2005

Inverse Square Law

Inverse Square Law

$$I_0 = \frac{I_S}{4\pi d^2}$$

$$I_d(x,y) = \frac{I_S}{4\pi r^2} \quad \text{where } r^2 = x^2 + y^2 + d^2$$

$$= \frac{I_0 d^2}{r^2} = I_0 \cos^2\theta$$



Prince and Links 2005

Obliquity Factor

Obliquity Factor

$I_d(x,y) = I_0 \cos\theta$

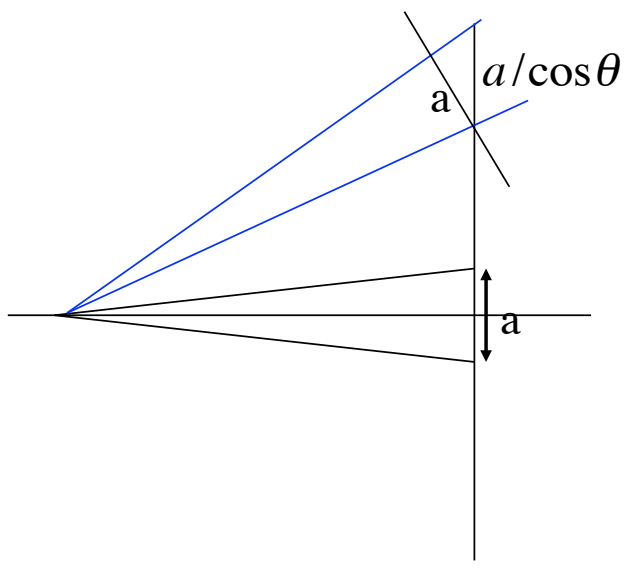



Prince and Links 2005

TT Liu, BE280A, UCSD Fall 2015

X-Ray Imaging Geometry

Beam Divergence and Flat Panel

$I_r = I_0 \cos^3\theta$

Example : Chest x - ray at 2 yards with 14x17 inch film.

Question : What is the smallest ratio I_r/I_0 across the film?

$$r_d = \sqrt{7^2 + 8.5^2} = 11$$

$$\cos\theta = \frac{d}{\sqrt{r_d^2 + d^2}} = 0.989$$

$$\frac{I_r}{I_0} = \cos^3\theta = 0.966$$

TT Liu, BE280A, UCSD Fall 2015

Path Length

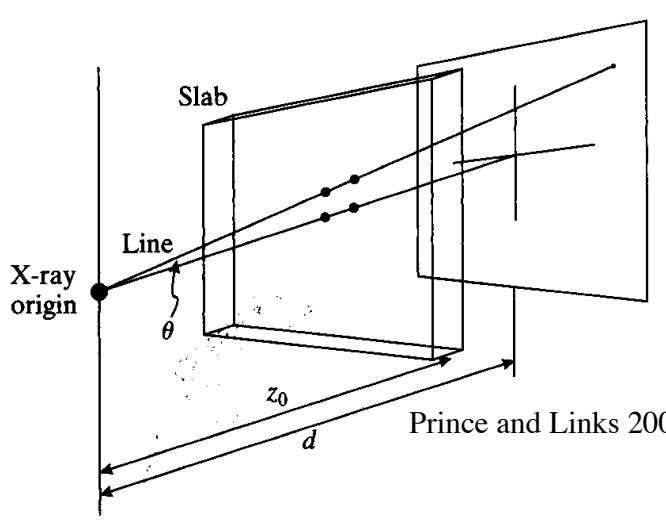

Prince and Links 2005

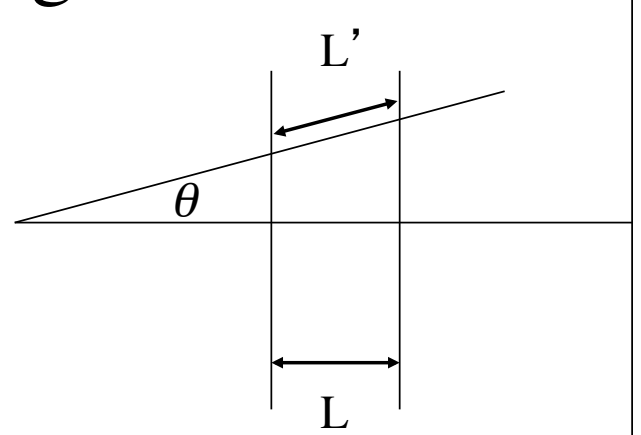

$$L' = L/\cos\theta$$

$$I_d(x,y) = I_0 \cos^3\theta \exp(-\mu L/\cos\theta)$$

TT Liu, BE280A, UCSD Fall 2015

Magnification of Object

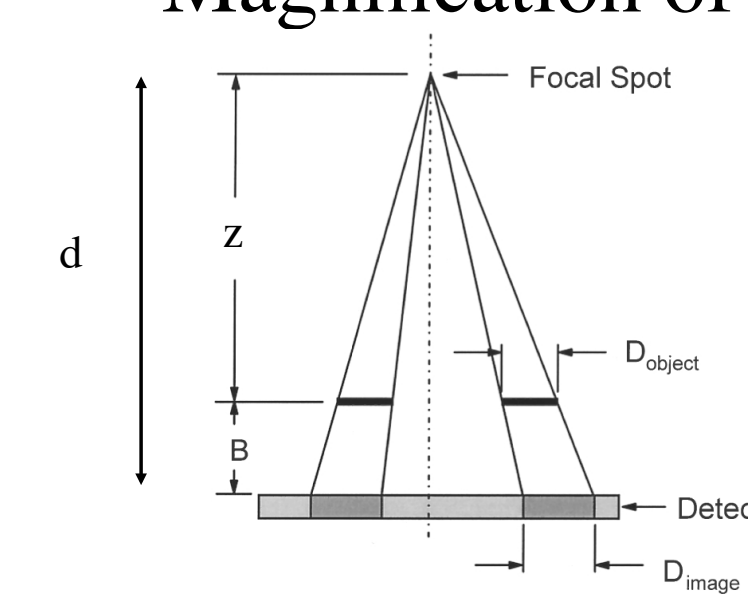

$$M(z) = \frac{d}{z}$$

$$= \frac{\text{Source to Image Distance (SID)}}{\text{Source to Object Distance (SOD)}}$$

TT Liu, BE280A, UCSD Fall 2015

Bushberg et al 2001

Magnification of Object

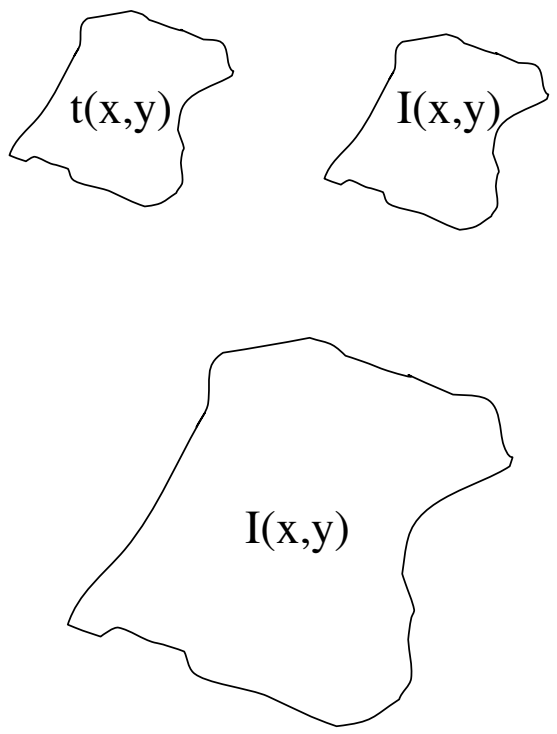

M = 1: I(x,y) = t(x,y)

M = 2: I(x,y) = t(x/2,y/2)

In general, I(x,y) = t(x/M(z),y/M(z))

Object Magnification

Question: All other things being equal, the optimal distance (z) between the source and the object is
a) 0
b) d/5
c) d/2
d) d
where d is the distance between the source and the detector.

PollEv.com/be280a

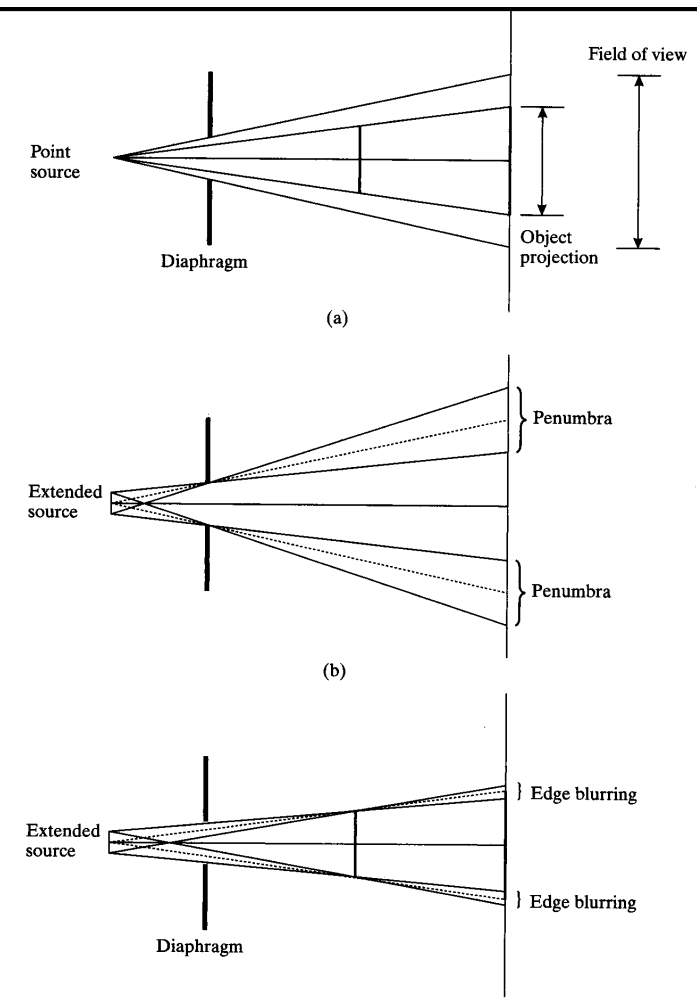

Prince and Link 2005

Figure 5.18
Effects of extended source. (a) Ideal field of view and object projection (with magnification). (b) Penumbra at edges of field of view due to extended source. (c) Blurred object edges due to extended source.

Source magnification

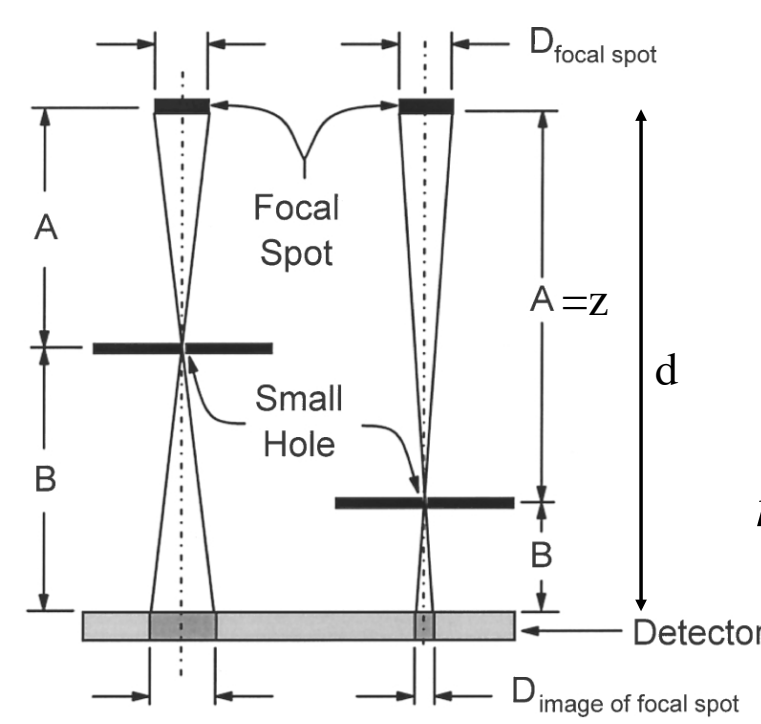

Bushberg et al 2001

$$\frac{D_{image}}{D_{focal}} = \frac{d-z}{z}$$

$$m(z) = -\frac{d-z}{z} = -\frac{B}{A}$$
$$= 1 - M(z)$$

Source Magnification

Question: All other things being equal, the optimal distance (z) between the source and the object for minimizing the effects of source magnification is:

a) 0
b) d/5
c) d/2
d) d

where d is the distance between the source and the detector.

PollEv.com/be280a

M=2
m=-1

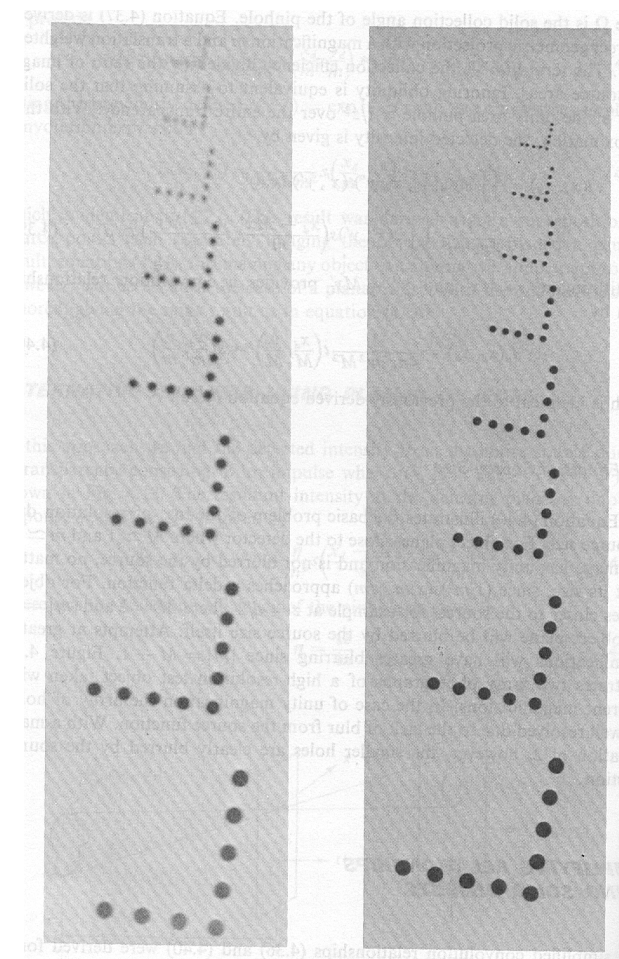

M=1
m=0

Macovski 1983

Rectangle Function

$$\Pi(x) = \begin{cases} 0 & |x| > 1/2 \\ 1 & |x| \le 1/2 \end{cases}$$



Also called rect(x)

$$\Pi(x,y) = \Pi(x)\Pi(y)$$

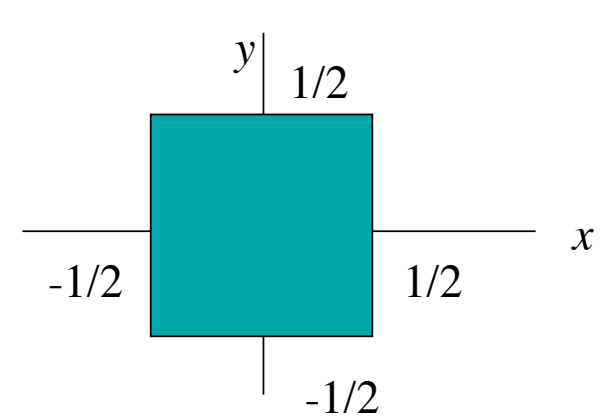

Dirac Delta Function

Notation:

$\delta(x)$ - 1D Dirac Delta Function

$\delta(x,y)$ or ${}^2\delta(x,y)$ - 2D Dirac Delta Function

$\delta(x,y,z)$ or ${}^3\delta(x,y,z)$ - 3D Dirac Delta Function

$\delta(\vec{r})$ - N Dimensional Dirac Delta Function

1D Dirac Delta Function

$\delta(x) = 0$ when $x \neq 0$ and $\int_{-\infty}^{\infty} \delta(x)dx = 1$

Can interpret the integral as a limit of the integral of an ordinary function that is shrinking in width and growing in height, while maintaining a constant area. For example, we can use a shrinking rectangle function

such that $\int_{-\infty}^{\infty} \delta(x)dx = \lim_{\tau \to 0} \int_{-\infty}^{\infty} \tau^{-1}\Pi(x/\tau)dx.$



Image of a point object

$I_d(x,y) = ks(x/m, y/m)$ Assume s(x,y) has unit area

$\int\int ks(x/m(z), y/m(z))dxdy =$ constant

$\Rightarrow k = \frac{1}{m^2(z)}$

$$I_d(x,y) = \lim_{m \to 0} \frac{s(x/m, y/m)}{m^2} = \delta(x,y)$$

X-Ray Imaging

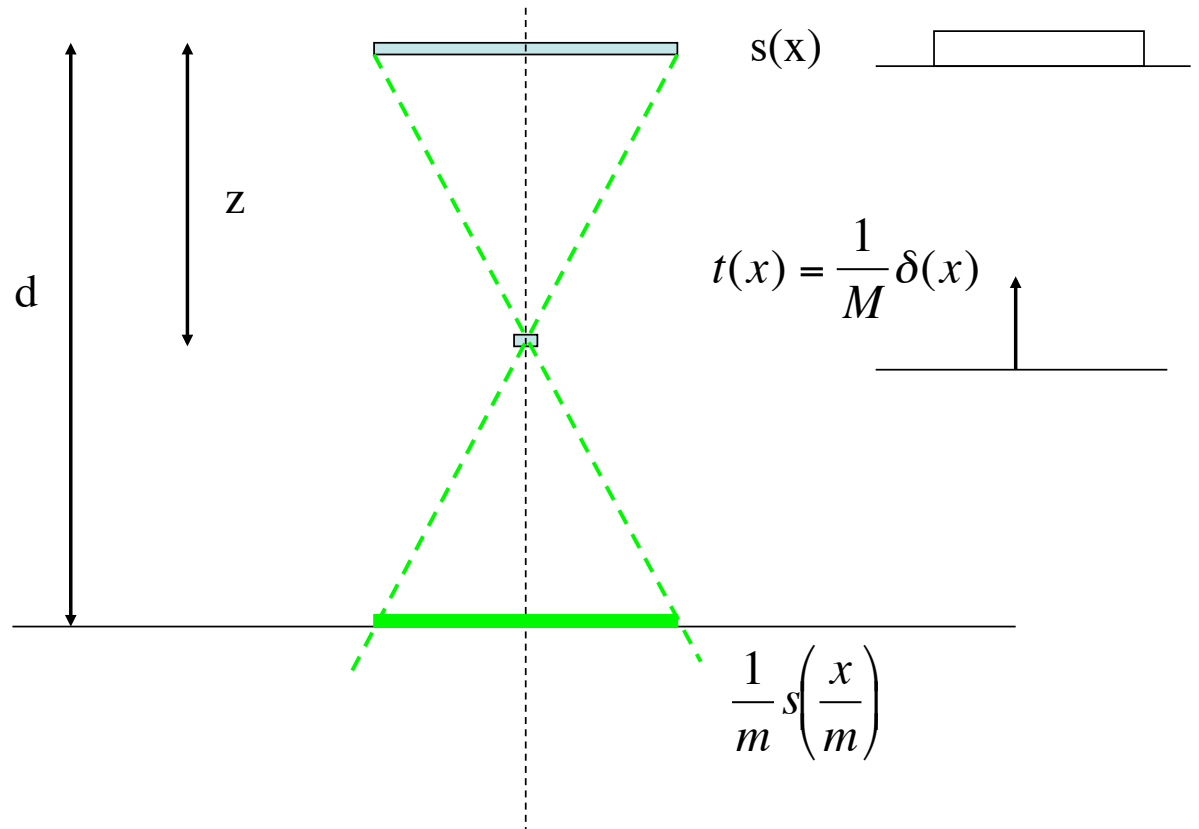

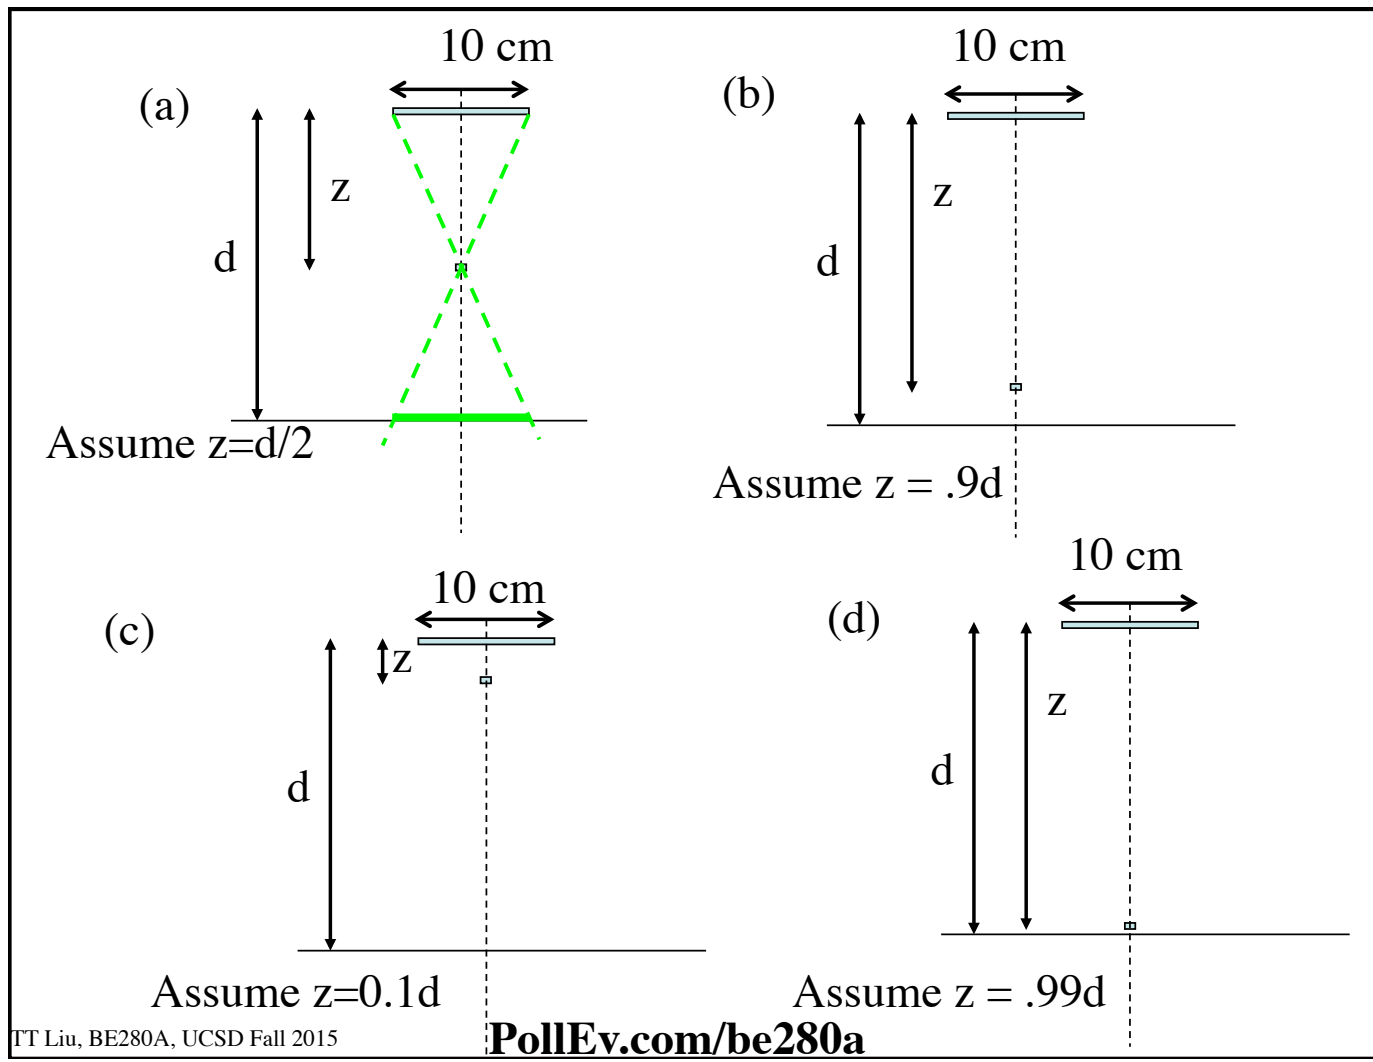

PollEv.com/be280a

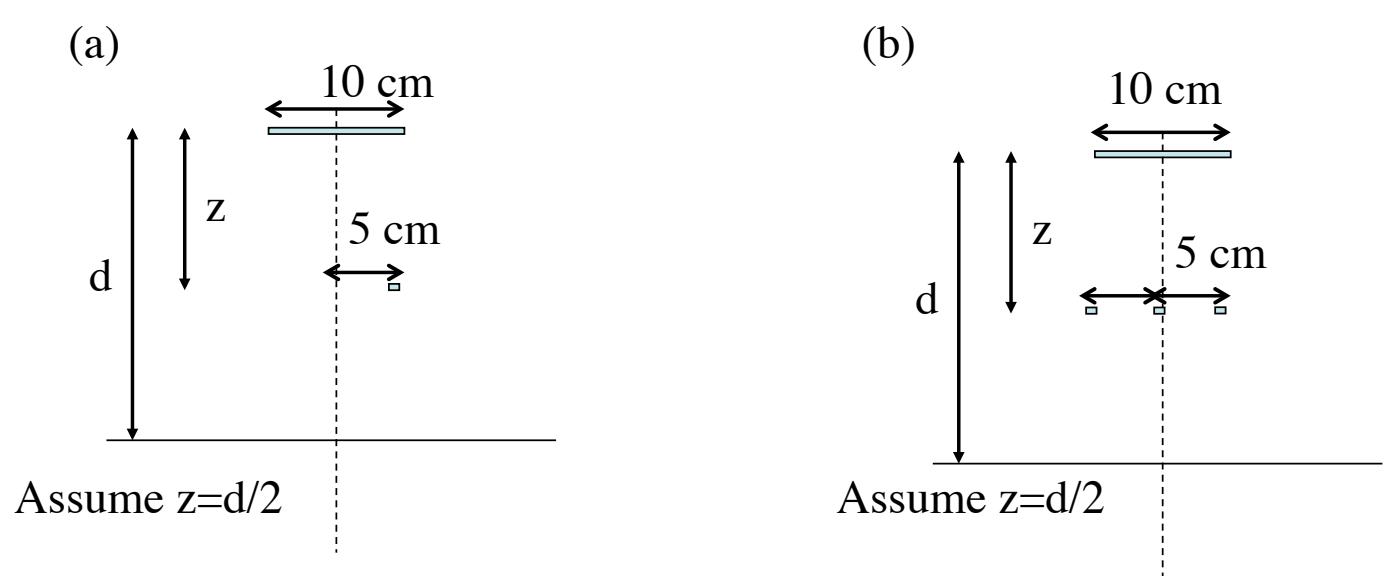

pollEv.com/be280a